

APPLICANT: JEFFREY M. SIERACKI ET AL
TITLE: FAILSAFE PROGRAMMING OF IMPLANTABLE MEDICAL DEVICES
ATTORNEY/AGENT: JASON D. KELLY
REG. NO. 54,213 TELEPHONE: 651.735.1100
DOCKET NO.: 1023-227US01 SHEET 1 OF 7

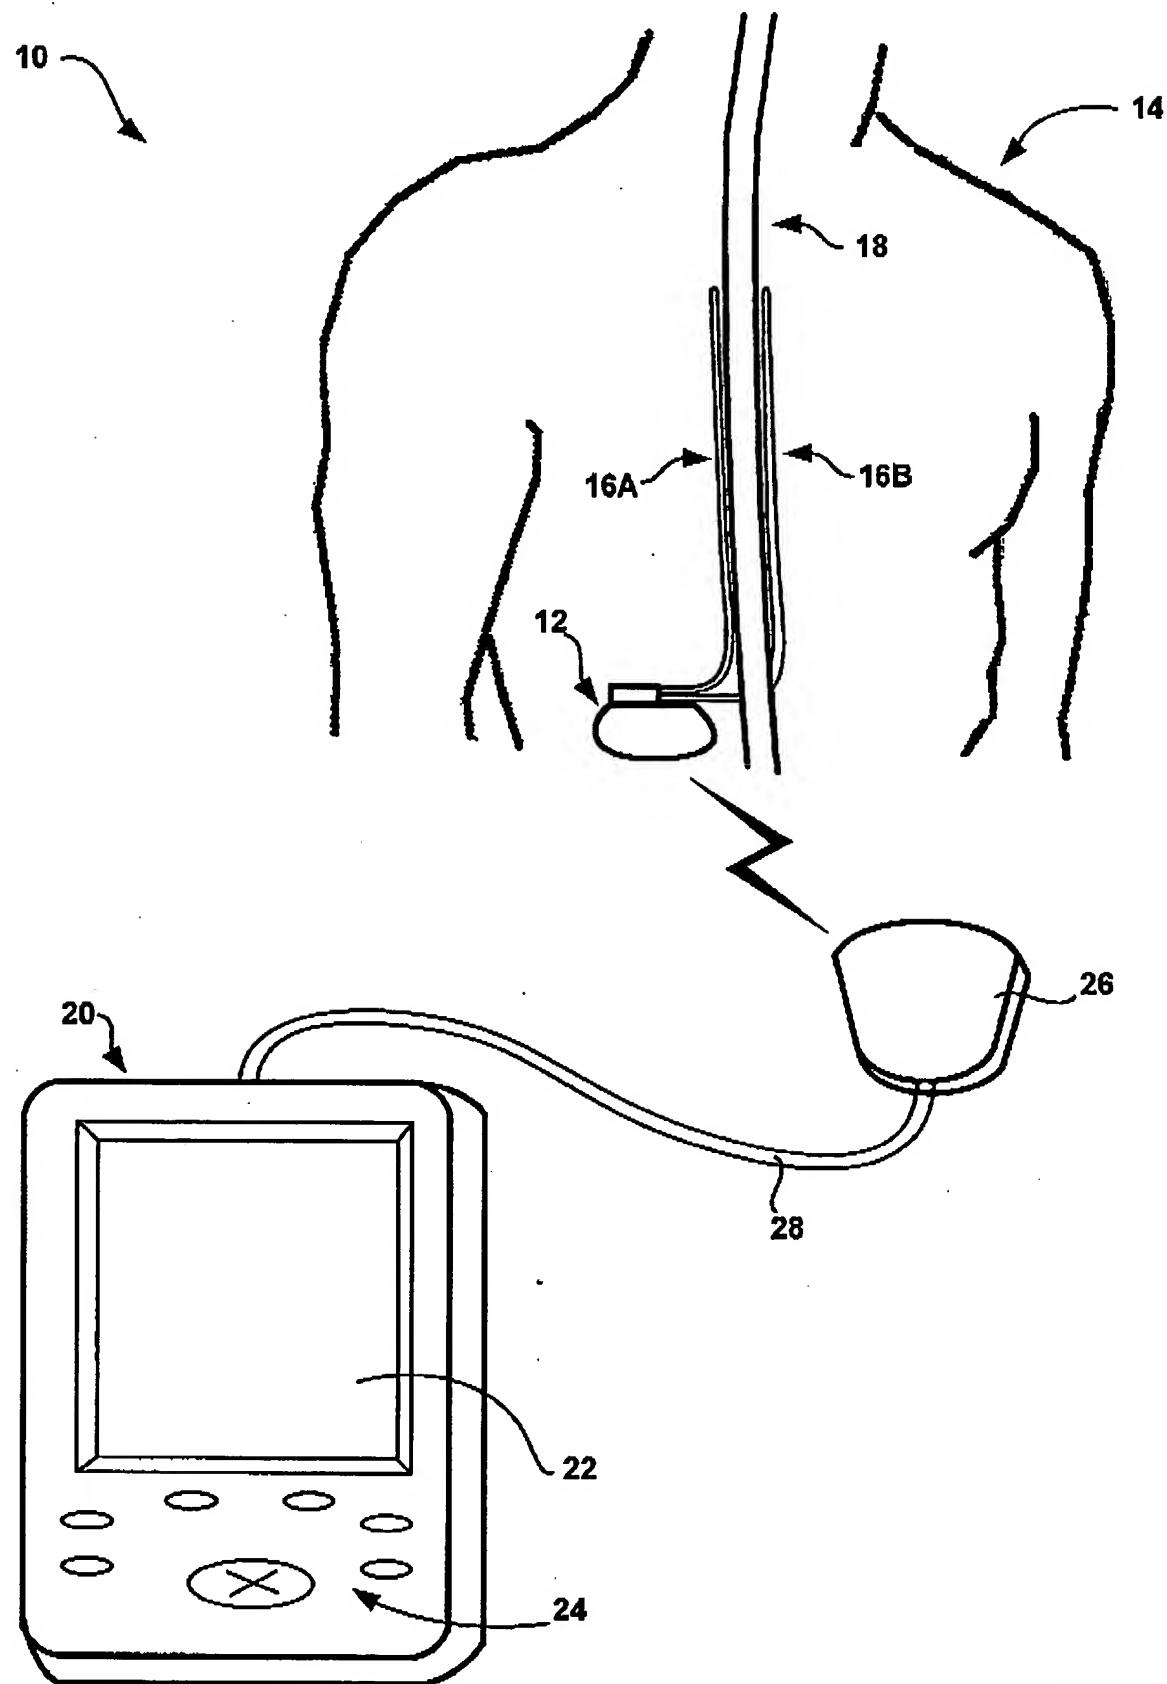


FIG. 1

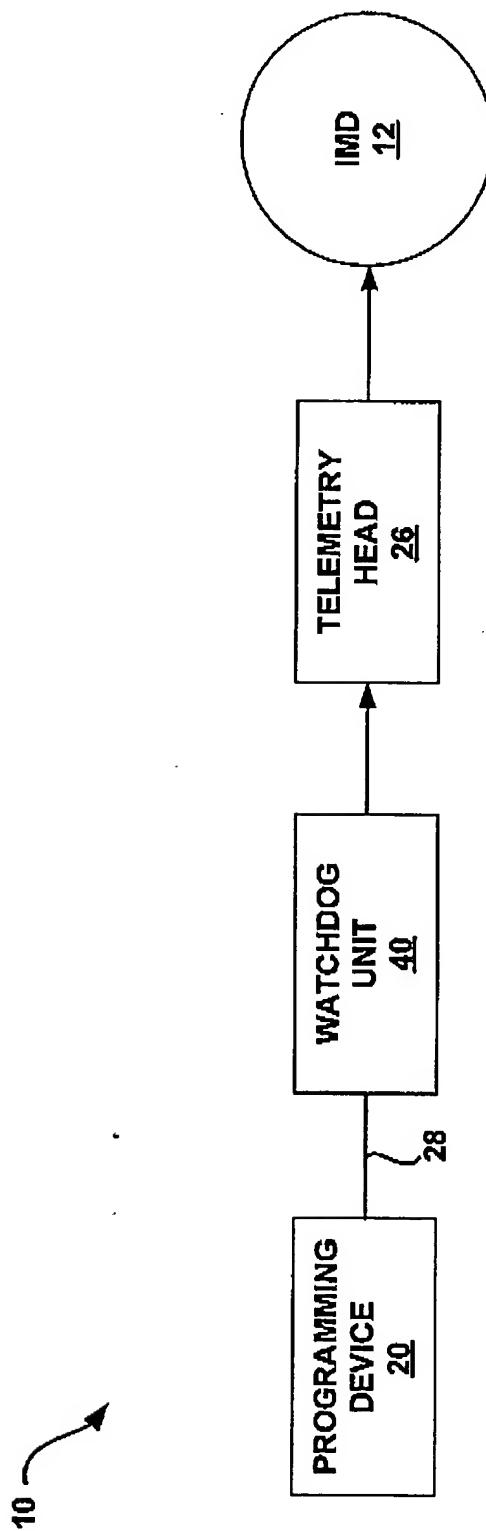


FIG. 2

APPLICANT: JEFFREY M. SIERACKI ET AL.
TITLE: FAILSAFE PROGRAMMING OF IMPLANTABLE MEDICAL DEVICES
ATTORNEY/AGENT: JASON D. KELLY
REG. NO. 54,213 TELEPHONE: 651.735.1100
DOCKET NO.: 1023-227US01 SHEET 3 OF 7

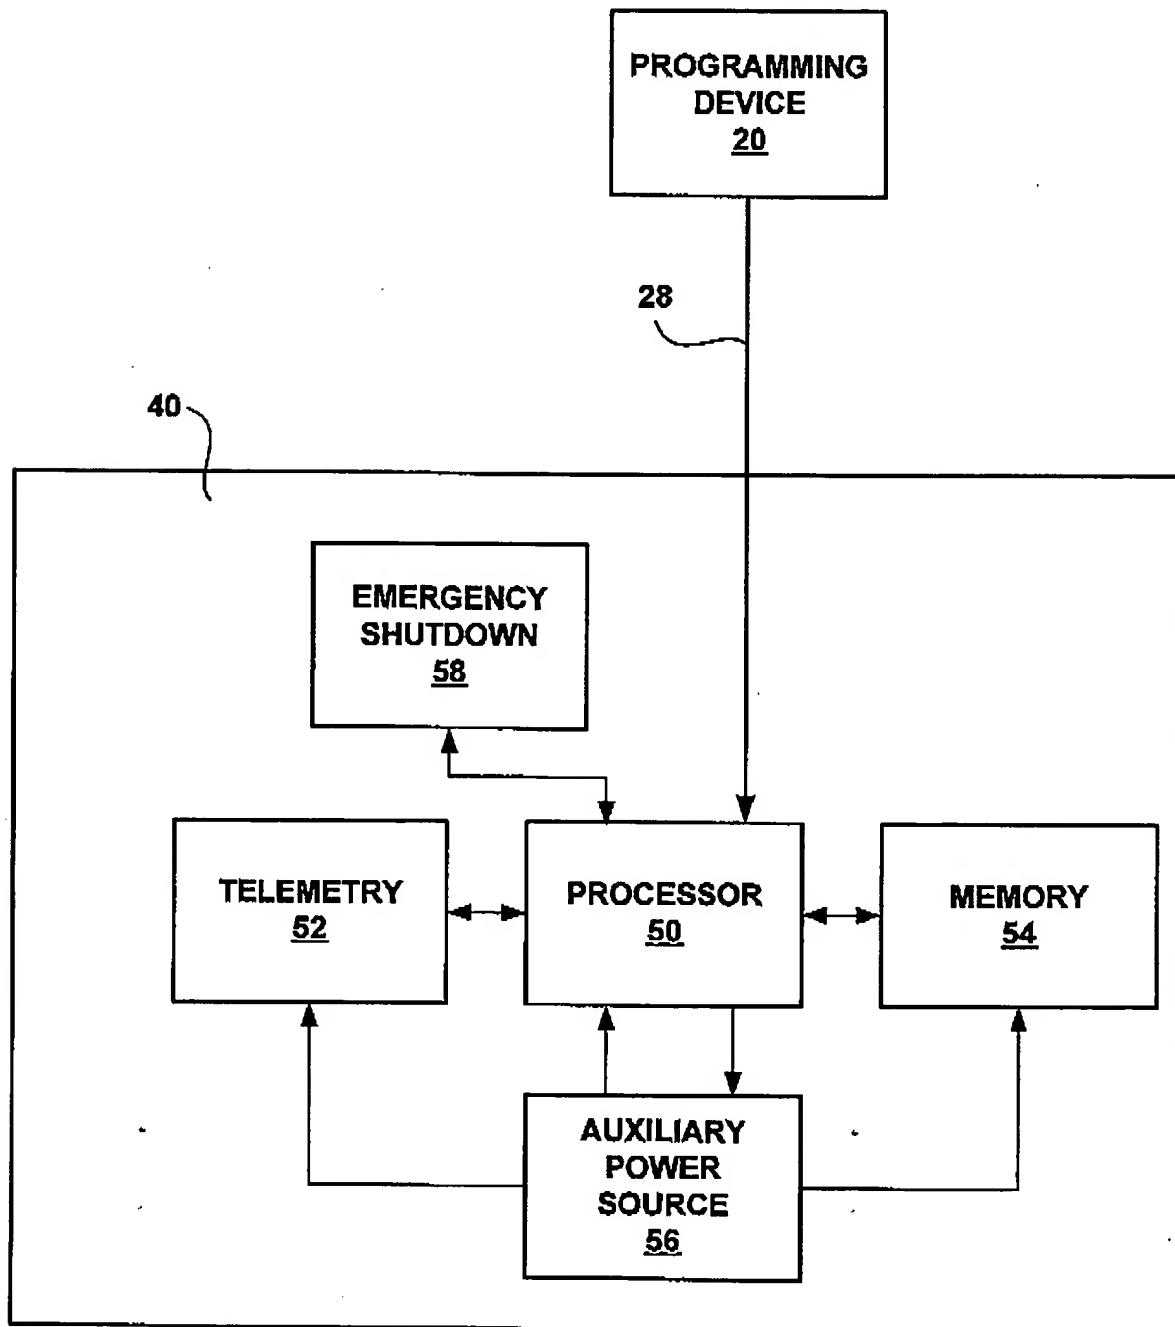


FIG. 3

APPLICANT: JEFFREY M. SIERACKI ET AL.
TITLE: FAILSAFE PROGRAMMING OF IMPLANTABLE MEDICAL DEVICES
ATTORNEY/AGENT: JASON D. KELLY
REG. NO. 54,213 TELEPHONE: 651.735.1100
DOCKET NO.: 1023-227US01 SHEET 4 OF 7

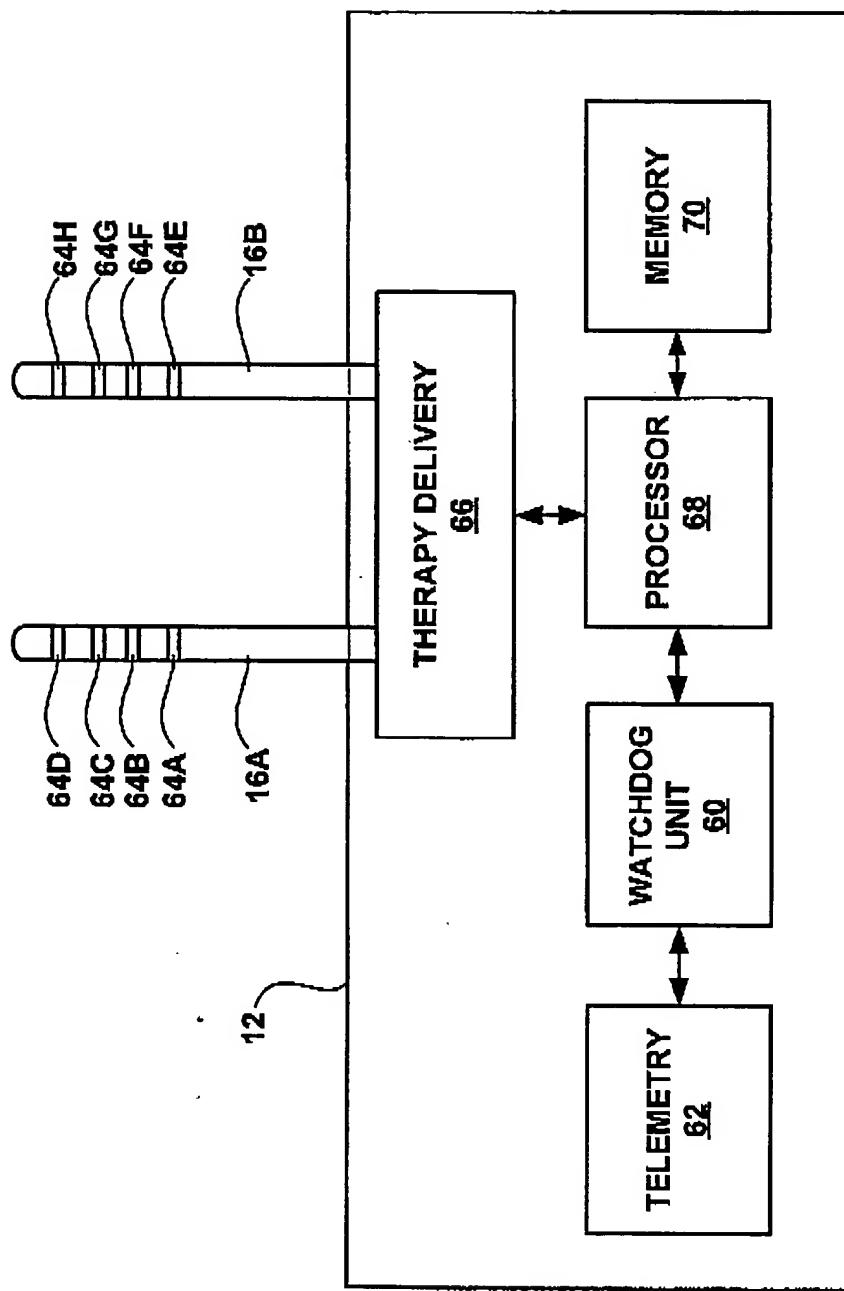


FIG. 4

APPLICANT: JEFFREY M. SIERACKI ET AL.
TITLE: FAILSAFE PROGRAMMING OF IMPLANTABLE MEDICAL DEVICES
ATTORNEY/AGENT: JASON D. KELLY
REG. NO. 54,213 TELEPHONE: 651.735.1100
DOCKET NO.: 1023-227US01 SHEET 5 OF 7

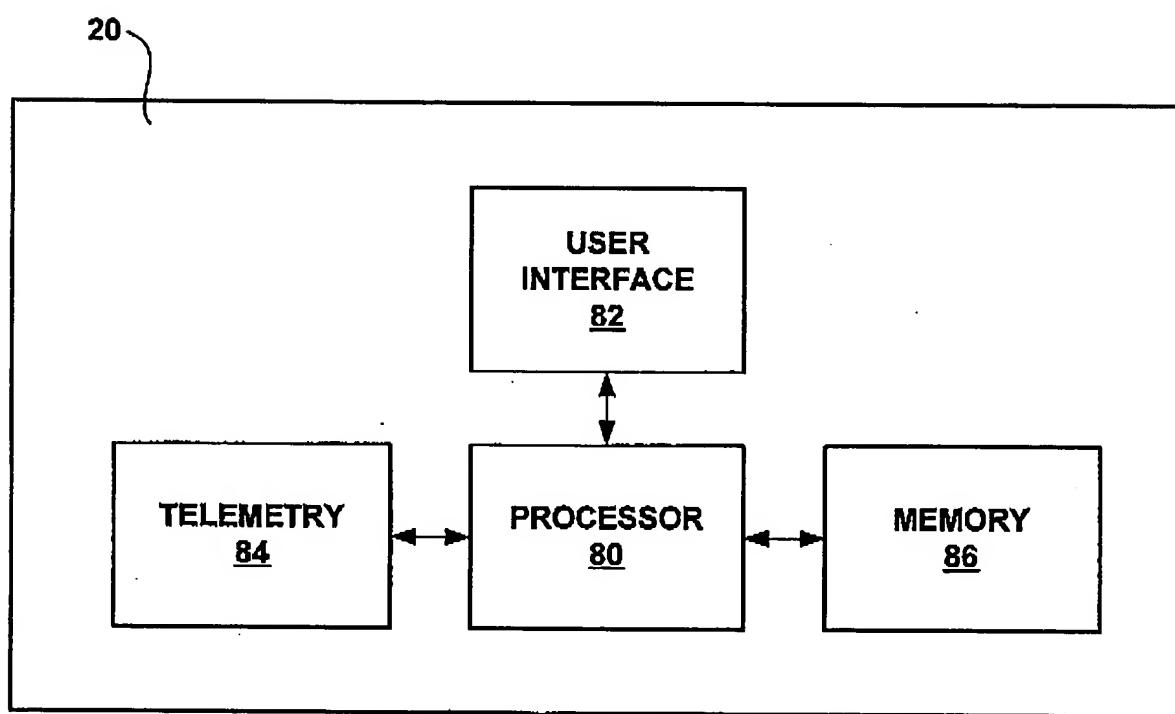


FIG. 5

APPLICANT: JEFFREY M. SIERACKI ET AL.
TITLE: FAILSAFE PROGRAMMING OF IMPLANTABLE MEDICAL DEVICES
ATTORNEY/AGENT: JASON D. KELLY
REG. NO. 54,213 TELEPHONE: 651.733.1100
DOCKET NO.: 1023-227US01 SHEET 6 OF 7

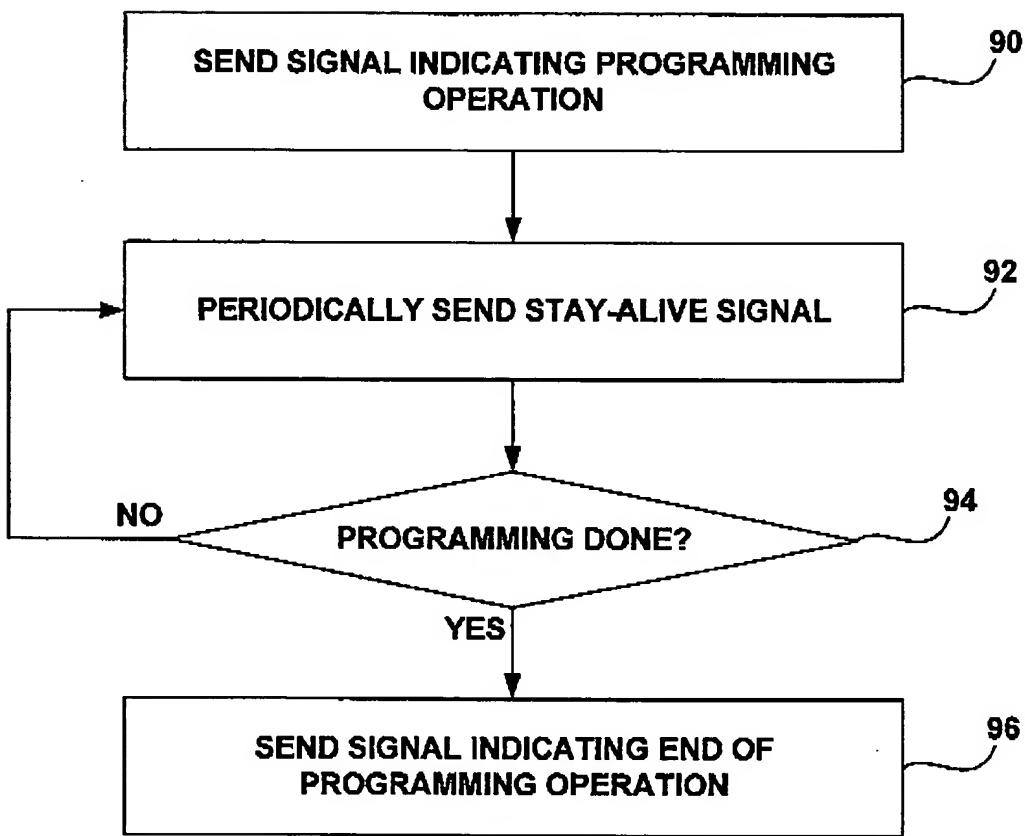


FIG. 6

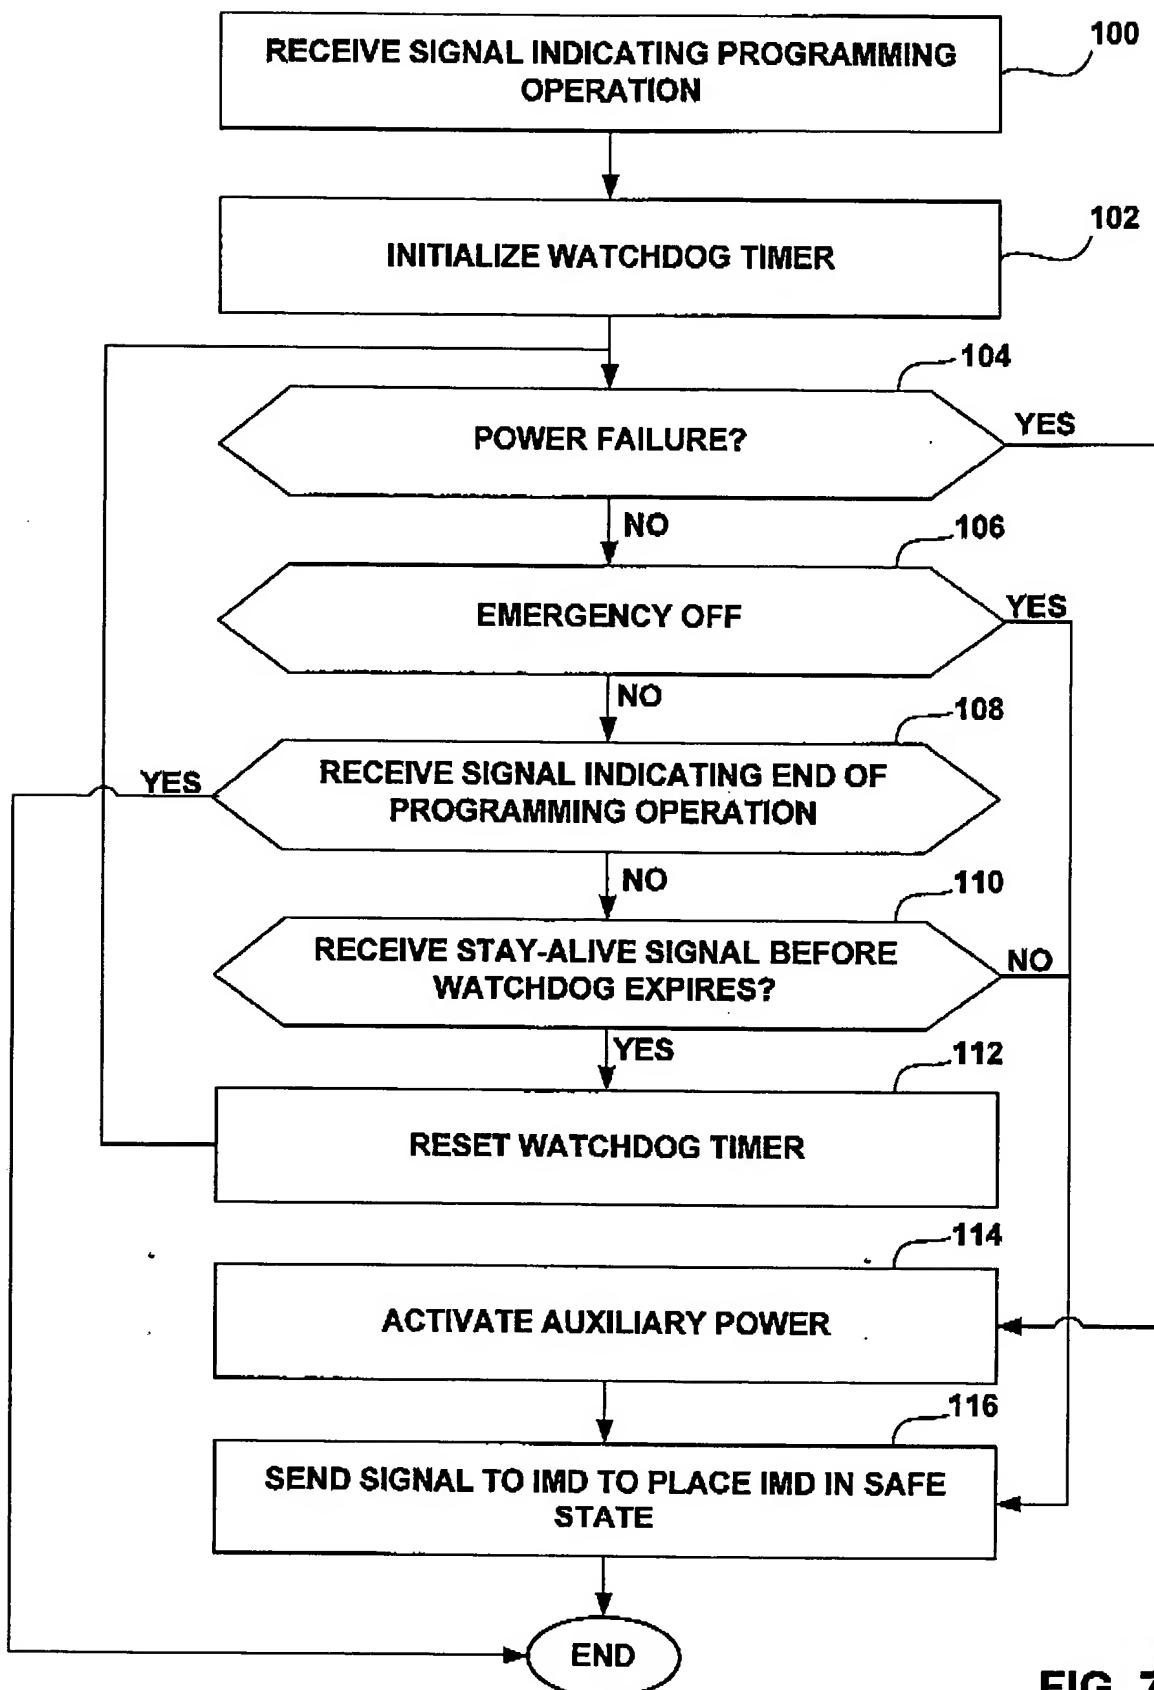


FIG. 7